

# MICRO-DOT™ MANUAL SYRINGE DISPENSER



## TRIDAK® MICRO-DOT

- Portable, hand-held dispenser with positive-displacement accuracy
- Accepts pre-packaged 10 cc syringes
- Dispenses a wide range of fluids from low-to-high viscosities
- Adjustable dot size
- Plastic taper tip recommended for most accurate dispensing
- Compact and light weight
- Lever or thumb pressure actuation

The Micro-Dot™ manual syringe dispenser combines the efficiency of disposable syringes with a precise, repeatable, reusable, manually-actuated delivery device. This hand-held syringe dispenser can be set to deliver volumes as small as 0.0003 mL. Once a volume is set it can be repeated indefinitely with extreme accuracy. The Micro-Dot™ is suitable for dispensing a wide range of low-to-high viscosity fluids.

**P/N T15473**

## SPECIFICATIONS:

### Dispenser Type:

Manual positive displacement

### Weight (without syringe):

2.8 oz (81.3 g)

### Dimensions:

4.5" L x .87" W x 2.125" H  
(114 mm x 22 mm x 54 mm)

### Shot Size:

Minimum: .0003 mL  
(400 cP material with 25 gauge taper tip)


Maximum: 0.170 mL  
(400 cP material with 14 gauge taper tip)

**Tridak**®

Precision Dispensing & Filling Equipment  
[www.tridak.com](http://www.tridak.com)

# MICRO-DOT™ MANUAL SYRINGE DISPENSER

## Micro-Dot™ with Thumb Actuation

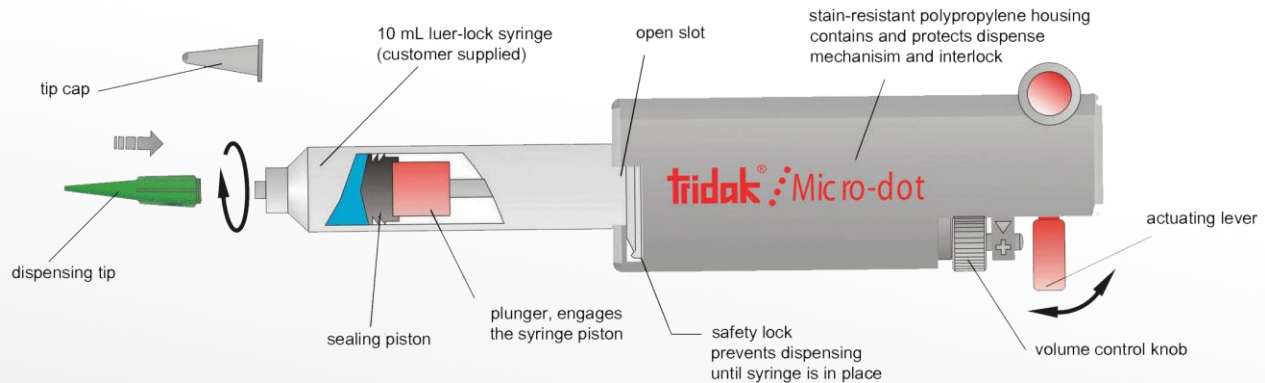

© 2009-2011 Tridak LLC. All rights reserved.

The data contained in this bulletin is of general nature and is based on laboratory test conditions. Tridak does not warrant the data contained in this bulletin. Any warranty applicable to the product, its application and use is strictly limited to that contained in Tridak's standard Conditions of Sale. Tridak does not assume responsibility for test or performance results obtained by users. It is the user's responsibility to determine the suitability for the product application and purposes and the suitability for use in the user's intended manufacturing apparatus and methods. The user should adopt such precautions and use guidelines as may be reasonably advisable or necessary for the protection of property and persons. Nothing in this bulletin shall act as a representation that the product use or application will not infringe a patent owned by someone other than Tridak or act as a grant of license under any Tridak LLC Patent. Tridak recommends that each user adequately test its proposed use and application before repetitive use, using the data contained in this bulletin as a general guide.

TRI014 10/2011